

1/8

FIG. 1A


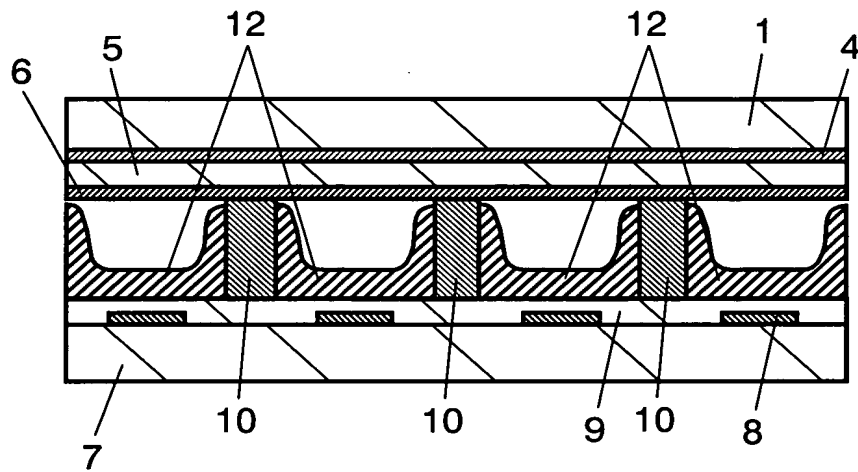


FIG. 1B

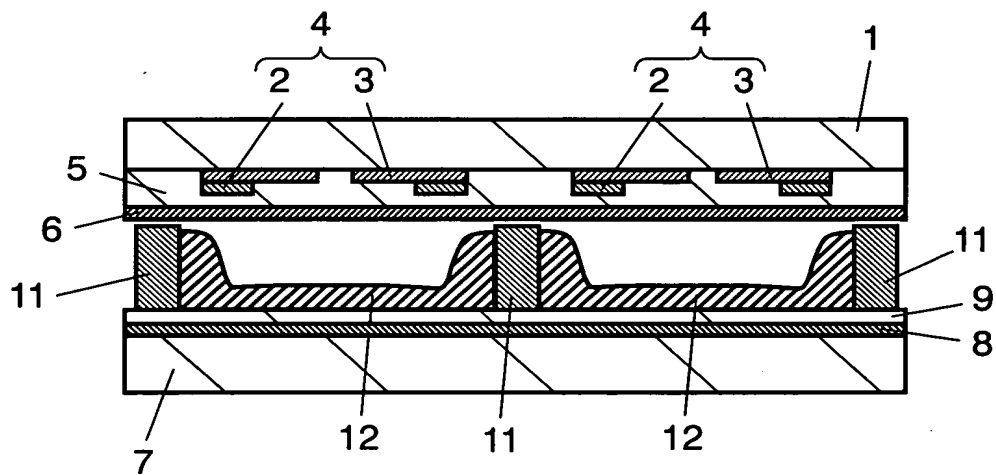

2/8

FIG. 2

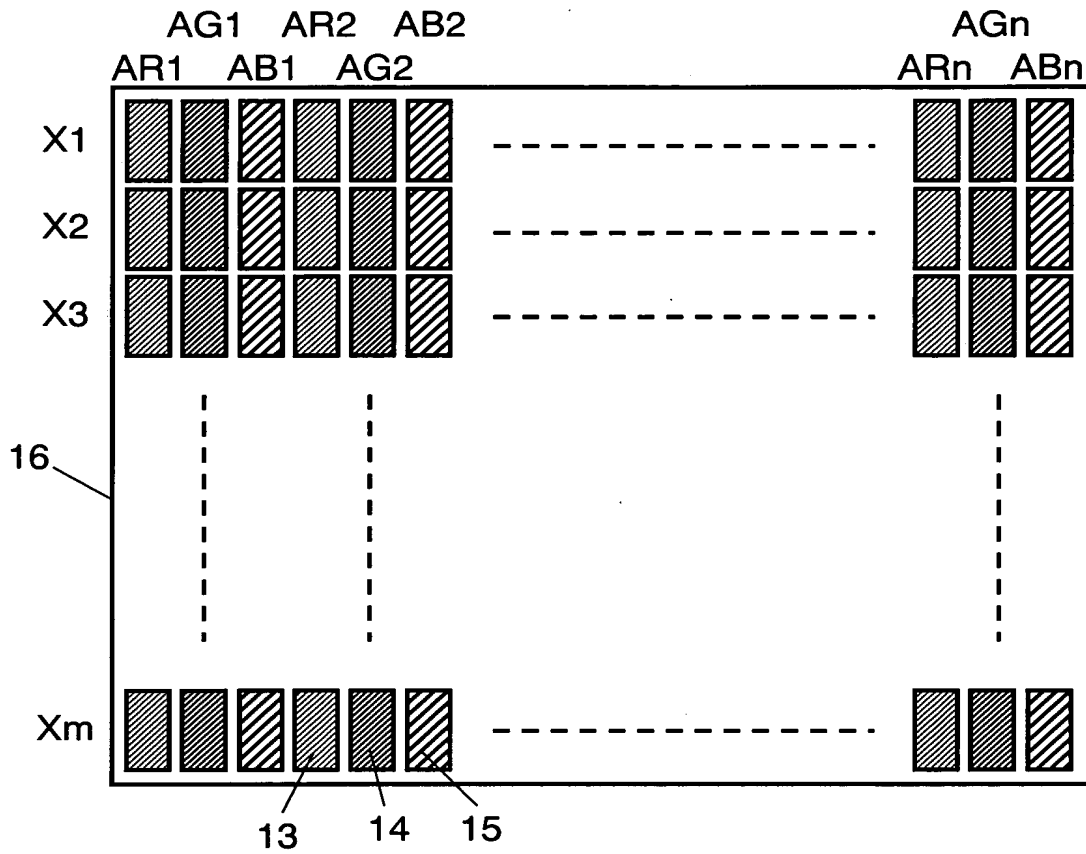


FIG. 3



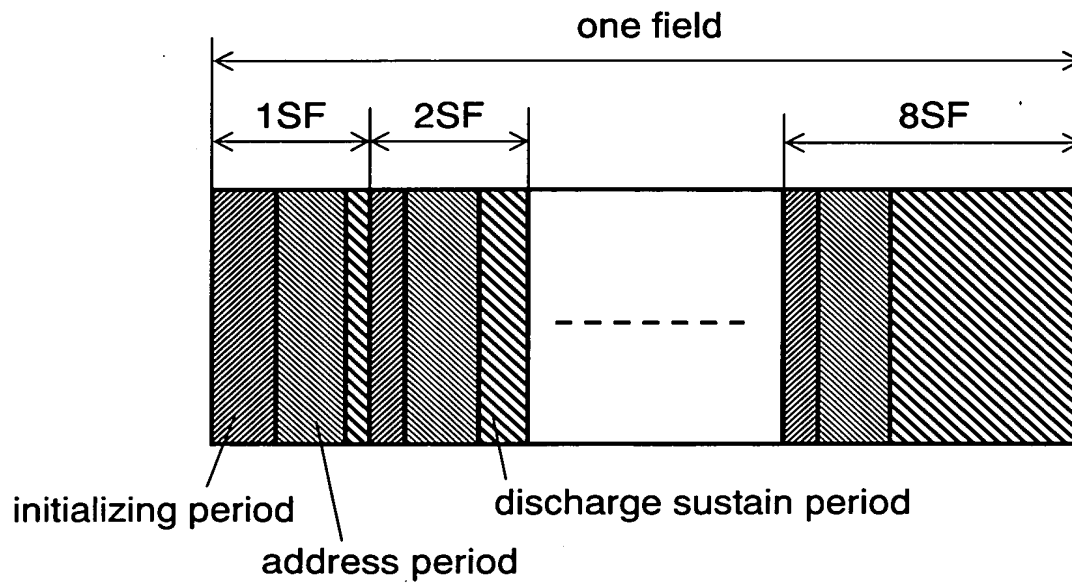


FIG. 4

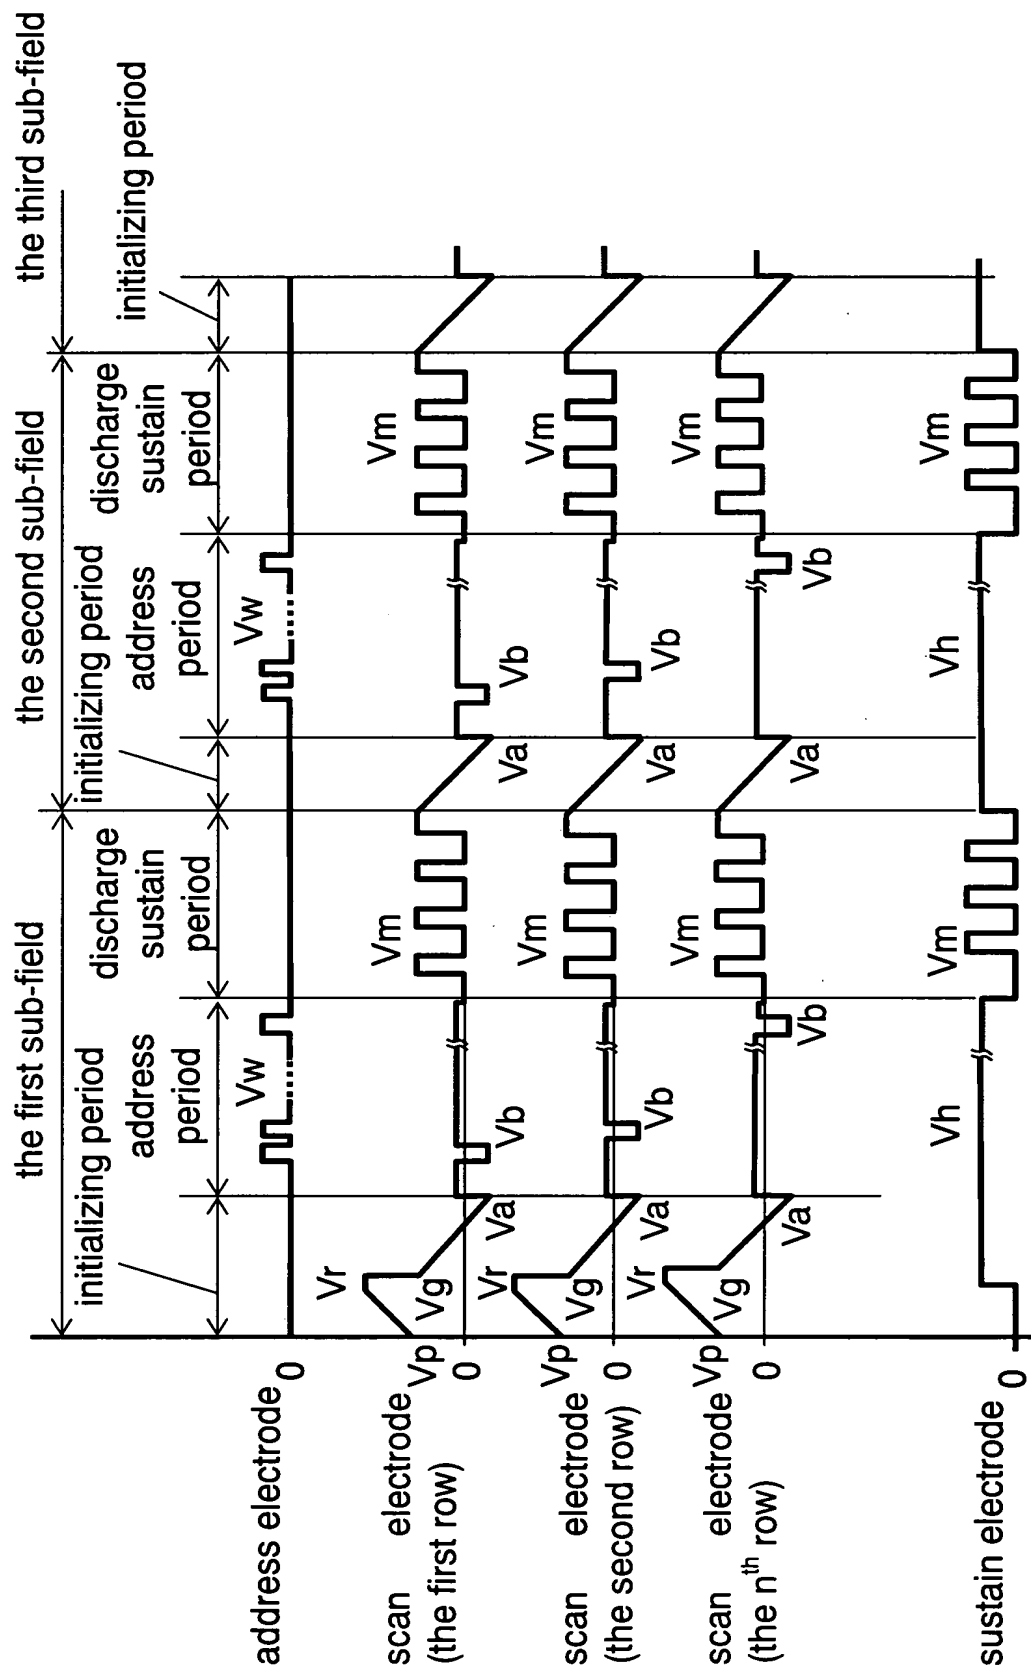

4/8

FIG. 5

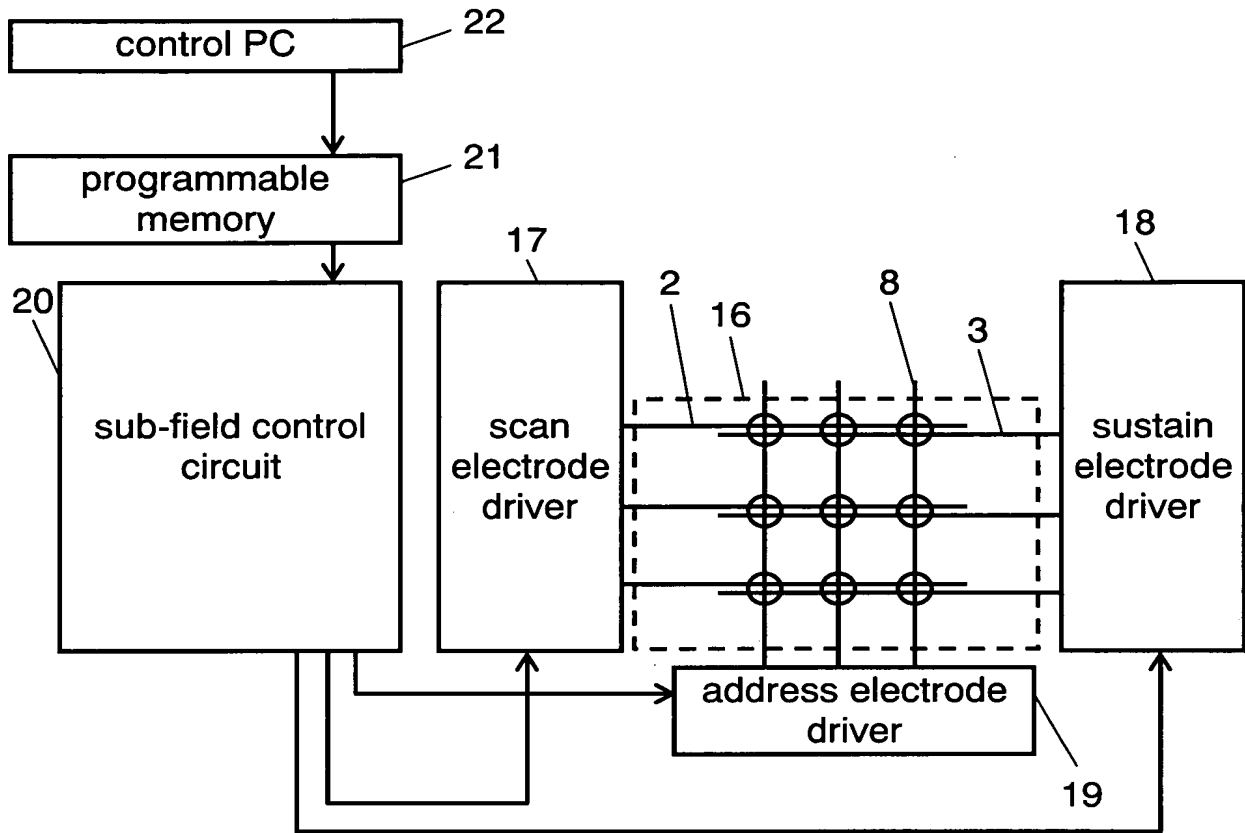

5/8

FIG. 6

R-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	○	○	○	×	×	×	×	×
even-rows	×	×	×	×	×	×	×	×

G-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	×	×	×	○	×	×	×	×
even-rows	×	×	×	×	×	×	×	×

B-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	○	○	○	×	×	×	×	×
even-rows	×	×	×	×	×	×	×	×

○ : address pulse is applied

× : address pulse is not applied

6/8

FIG. 7

R-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	x	x	x	x	x	x	x	x
even-rows	x	x	x	x	x	x	x	x

G-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	○	○	○	x	x	x	x	x
even-rows	x	x	x	○	x	x	x	x

B-cell

rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
odd-rows	x	x	x	x	x	x	x	x
even-rows	x	x	x	x	x	x	x	x

○ : address pulse is applied

x : address pulse is not applied

7/8

FIG. 8

R-cell	rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
	odd-rows	○	○	○	×	×	×	×	×
	even-rows	×	×	×	×	×	×	×	×

G-cell	rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
	odd-rows	×	×	×	×	×	×	×	×
	even-rows	×	×	×	○	×	×	×	×

B-cell	rows	1SF	2SF	3SF	4SF	5SF	6SF	7SF	8SF
	odd-rows	○	○	○	×	×	×	×	×
	even-rows	×	×	×	×	×	×	×	×

○ : address pulse is applied

× : address pulse is not applied

8/8

Reference numerals in the drawings

- 2: scan electrode
- 3: sustain electrode
- 4: display electrode
- 8: address electrode
- 13: R-cell
- 14: G-cell
- 15: B-cell